



## NOTE

### Determination of Sodium Chloride in Crude Oil of Gachsaran County Oil Wells

R. HAJIAN<sup>1\*</sup>, A.H. OROOJLOO<sup>2</sup>, S.S. MOUSAVIAN<sup>2</sup> and N. SHAMS<sup>2</sup>

<sup>1</sup>Young Researchers Club, College of Science, Chemistry Department, Islamic Azad University Branch of Gachsaran, Gachsaran 75818-63876, Iran

<sup>2</sup>College of Science, Chemistry Department, Islamic Azad University Branch of Gachsaran, Gachsaran, 75818-63876, Iran

\*Corresponding author: Fax: +98 742 3334750; Tel: +98 742 3334751; E-mail: hajian@iaug.ac.ir

(Received: 16 September 2010;

Accepted: 30 May 2011)

AJC-10008

A new automated liquid-liquid extraction (LLE) apparatus have been designed and the applicability of this device was tested by the analysis of sodium chloride in crude oil of Gachsaran region in south of Iran. All of the results were compared with the standard test method. The advantages of this device include portability, water reservoir, cooling system, temperature controller and water level controller. The statistical test methods including t-test and F-test showed good accuracy and precision respectively in the analysis of sodium chloride in crude oils. The results showed that the mean of salt concentration as sodium chloride were  $31.0 \text{ g m}^{-3}$  with the relative standard deviation of (% RSD) 7.9 in Gachsaran county oil wells.

**Key Words:** Sodium chloride, Liquid-liquid extraction, Crude oil, Gachsaran region.

Many processes in chemical engineering require the separation of one or more of the components of a liquid mixture by treating the mixture with an immiscible solvent in which these components are preferentially soluble<sup>1</sup>. In some cases purification of a liquid may be the function of the process, in others the extraction of a dissolved component for subsequent processes may be the important aspect. An example of the former is the preparation of the pure organic liquids from products of the oil industry. Liquid-liquid extractions may also be used as energy saving processes by, for example, eliminating distillation stages. It is possible, of course that the substance of interest may be heat-sensitive anyway and that distillation is accordingly an unacceptable process<sup>2</sup>.

When separation by distillation is ineffective or very difficult, liquid extraction is one of the main alternatives to consider. Close-boiling mixtures or substances that cannot withstand the temperature of the distillation, even under a vacuum, may often be separated from impurities by extraction, which utilizes chemical differences instead of vapour pressure differences. For example, penicillin is recovered from fermentation broth by extraction with a solvent such as butyl acetate. Another example for liquid extraction is recovering acetic acid from dilute aqueous solutions; distillation would be possible in this case, but the extraction step considerably reduces the amount of water to be distilled<sup>3</sup>.

Analysis of the sodium chloride content of crude oil is important because this allows the oil to be evaluated for poten-

tial to corrode equipment and pipelines. Salt measurements are taken along the supply line from well head to Refinery, rapid sample determination allows prompt corrective action when unacceptable levels of salt are present.

In the present work a reliable and portable liquid-liquid extraction apparatus have constructed involving water reservoir, cooling system, temperature controller and water level controller (Fig. 1). The applicability of the method was evaluated by the extraction of sodium chloride to aqueous phase and measured by the reversed titration using Volhard method.

All the chemicals were of analytical grade and were purchased from Fluka unless stated otherwise. Double distilled water was used throughout. A  $5.0 \times 10^{-2} \text{ mol L}^{-1}$  potassium thiocyanate solution was prepared by dissolving 0.4859 g potassium thiocyanate (99.5 %) in water and the solution was diluted to 100 mL with water in a 100 mL volumetric flask.

**Recommended procedure:** According to the standard test method (ASTM 2038), an amount of 80 g of crude oil was poured into a 250 mL glass balloon and heated to 60 °C. Then 40 mL toluene was heated to the same temperature and added to the glass balloon slowly. After that 25 mL ethanol and 15 mL acetone added to the solution and boiled for 12 min. After cooling at ambient temperature, the aqueous layer was filtered and separated to a flask. About 100 mL of the filtered aqueous layer was separated and acidified with 5 mL nitric acid (65 %). After removing of hydrogen sulphide completely, 100 mL amyl alcohol and 3 mL ferric alum added to the solution. Then, the

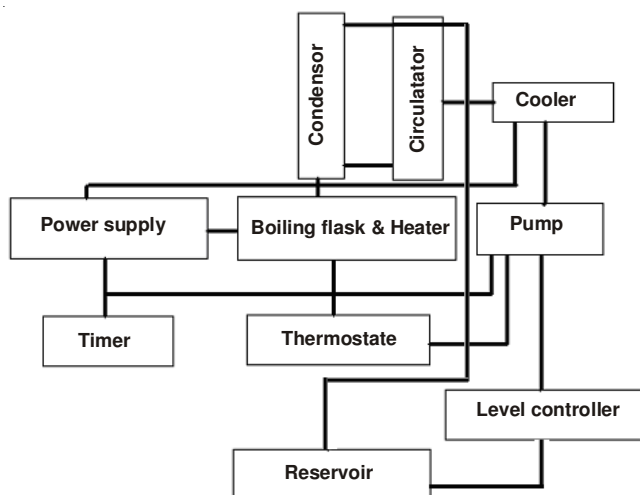


Fig. Liquid-liquid extraction apparatus

concentration of salt as sodium chloride was determined based on the Volhard method using potassium thiocyanate as the titrant.

**Reproducibility:** To check the reproducibility of the new liquid-liquid extraction apparatus, analysis of salt in crude oil was repeated for 5 times (Table-1). As it is shown, the recommended apparatus and procedure has good reproducibility.

Sample	Date	Sodium chloride (g m <sup>-3</sup> )	Mean (g m <sup>-3</sup> )	RSD (%)
Crude oil	24-02-2010	33.0	31.0	7.9
	25-02-2010	33.0		
	26-02-2010	28.0		
	27-02-2010	33.0		
	28-02-2010	28.0		

### Statistical tests

**t-test:** In order to compare the accuracy of the liquid-liquid extraction apparatus with older models, the analysis of sodium chloride in crude oil was replicate five times with each apparatus (Table-2).

Sample	Date	Sodium chloride (g m <sup>-3</sup> )	
		System 1*	System 2**
Crude oil	31-01-2010	23.0	28.0
	02-02-2010	28.0	23.0
	03-02-2010	23.0	23.0
	04-02-2010	37.0	35.0
	05-02-2010	28.0	28.0

\*Older liquid-liquid extraction apparatus.

\*\*Constructed liquid-liquid extraction apparatus.

**F-test:** The F-test is designed to test if two population variances are equal. It does this by comparing the ratio of two variances. In this research, a liquid-liquid extraction apparatus have designed with the advantages including water reservoir, cooling system, temperature controller and water level controller. Because of the water circulation in condenser, it is a powerful instrument as a portable extractor.

The applicability of this system have evaluated in the salt analysis of crude oil in Gachsaran Oil and Gas Producing Company. The results of the t-test ( $t_{cal} < t_{crit}$ ) shows good agreement between two systems (Table-3). The results of F-test on the replicate sodium chloride analyses (Table-4) showed a good precision between two extraction apparatuses ( $F_{cal} < F_{crit}$ ).

TABLE-3  
RESULTS OF t-TEST (WITH DIFFERENT SOURCE VARIANCES) BETWEEN THE RESULTS OF SODIUM CHLORIDE ANALYSIS IN CRUDE OIL BY TWO DIFFERENT EXTRACTION APPARATUS

Sources	Variable 1	Variable 2
Mean	25	25.4
Variance	9	9.8
Observations	5	5.0
Hypothesized mean difference	0	
df	8	
t Stat	0.210	
P (T<=t) one-tail	0.421	
t Critical one-tail	1.860	
P (T<=t) two-tail	0.840	
t Critical two-tail	2.310	

TABLE-4  
RESULTS OF F-TEST (CONFIDENCE LEVEL 95 %) FOR COMPARING THE PRECISION OF TWO EXTRACTION APPARATUSES

Sources	Variable 1	Variable 2
Mean	25.0	25.4
Variance	9.0	9.8
Observations	5.0	5.0
df	4.0	4.0
F	1.19	
P(F<=f) one-tail	0.05	
F Critical one-tail	6.39	

### ACKNOWLEDGEMENTS

The authors gratefully acknowledged the support of this work by Islamic Azad University branch of Gachsaran (IAUG). Also the assistance of The Gachsaran Oil & Gas Producing Company is gratefully acknowledged.

### REFERENCES

- C.O. Bennett and J.E. Myers, Momentum, Heat and Mass Transfer, McGraw-Hill, edn. 3 (1983).
- R.H. Perry and D. Green, Perry's Chemical Engineering Handbook, McGraw-Hill, edn. 6 (1984).
- R.K. Sinnott, J.M. Coulson and J.F. Richardson, An Introduction to Chemical Engineering Design, Pergamon Press, edn. 1 (1983).